


- **Stability in 100% aqueous mobile phase**
- **Outstanding reproducibility**
- **Highly pure, high surface area silica**
- **Highly inert towards basic compounds**
- **Rigorously tested to ensure quality**

Thermo Scientific Synchronis aQ HPLC Columns

Consistent, predictable separations,
Column after column, time after time


Specifications

Particle size	1.7 μm , 5 μm	Carbon load	19 %
Pore size	100 \AA	Endcapped	Polar
Surface area	320 m^2/g	USP classification	L1
pH range	2 - 8		



Stability in 100% aqueous mobile phase


In comparison to a conventionally endcapped C18, the Synchronis™ aQ polar end-capped C18 stationary phase exhibits superior stability towards aqueous mobile phase. Synchronis aQ shows no degradation in performance after 100 injections in a buffered 100% aqueous eluent.

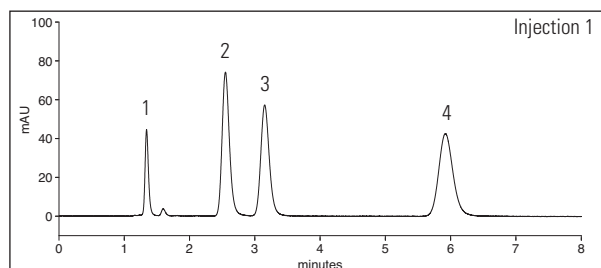

Column: Synchronis aQ, 5 μm , 100mm x 4.6mm

Mobile phase:	50mM Aqueous K_2HPO_4 (pH 6)
Flow rate:	0.7 mL/min
Temperature:	30°C
Detection:	260 nm
Injection volume:	2 μL


1. Cytidine-5'-diphosphate
2. Adenosine-5'-triphosphate
3. Adenosine-5'-diphosphate
4. Adenosine-5'-monophosphate

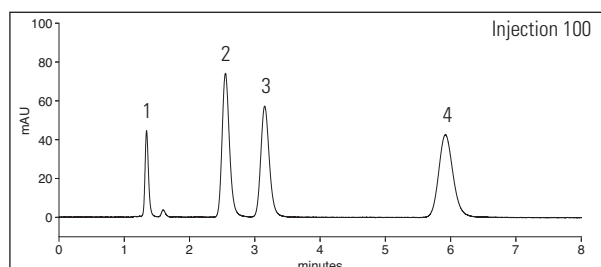

Stability of Synchronis aQ in 100% aqueous mobile phase

Description	Particle size	Length (mm)	2.1 mm ID	3 mm ID	4 mm ID	4.6 mm ID
Synchronis aQ	1.7 µm	30	97302-032130	–	–	–
		50	97302-052130	97302-053030	–	97302-054630
		100	97302-102130	97302-103030	–	–
	5 µm	30	97305-032130	97305-033030	97305-034030	97305-034630
		50	97305-052130	97305-053030	97305-054030	97305-054630
		100	97305-102130	97305-103030	97305-104030	97305-104630
Drop-in guard cartridges (4/pk)	5 µm	10	97305-012101	97305-013001	97305-014001	–

Application: Amoxicillin and Potassium Clavulanate (USP)

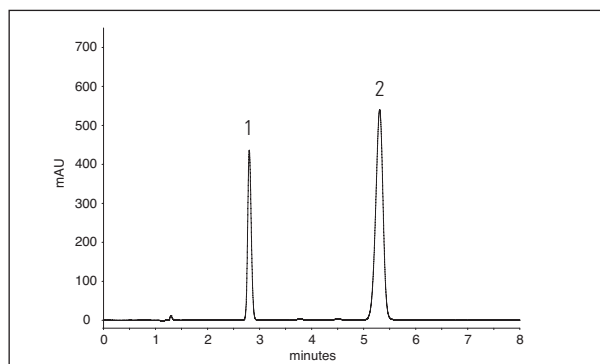

Column: Synchronis aQ, 5µm, 300mm x 4.0mm

Mobile phase: Phosphate Buffer (pH 4.4):
MeOH (95:5)

Flow rate: 2.0 mL/min

Temperature: 25°C

Detection: 210 nm

Injection volume: 20 µL

1. Amoxicillin
2. Potassium Clavulanate

Parameter	USP Specification	Measured Amoxicillin (6 replicate injections)	Measured K Clavulanate (6 replicate injections)
Resolution	> 3.5	–	12.8
Efficiency (N)	> 550	7598	6475
Tailing factor	< 1.5	1.15	0.92
%RSD Retention time	< 2%	0.29%	0.36%
%RSD Peak area	< 2%	0.30%	0.29%

Consistent, predictable separations, Column after column, time after time

Synchronis HPLC columns are manufactured, packed and tested in ISO9000 accredited facilities. Each lot of silica is tested for the physical properties of the silica support and only released for production if it meets the stringent test specifications.

Each bonded lot of chromatographic packing material is rigorously tested for primary and secondary interactions with the bonded phase.

New, enhanced, automated packing methods drive consistency even further and every column is individually tested to ensure that it meets the required quality.

These extensive testing and quality control procedures ensure the delivery of a consistent product, column after column.

For more information, visit www.thermoscientific.com/Synchronis

©2010 Thermo Fisher Scientific Inc. All rights reserved. All trademarks are the property of Thermo Fisher Scientific Inc. and its subsidiaries. Specifications, terms and pricing are subject to change. Not all products are available in all countries. Please consult your local sales representative for details.

SSCCSSYNCRONISAQ 0810

USA and Canada +1 800 332 3331

France +33 (0) 3 88 67 53 20

Germany +49 6103 408 0

Switzerland +41 56 618 41 11

United Kingdom +44 (0) 1928 534 110

Japan +81 45 453 9220

China +86-21-68654588 or +86-10-84193588

India 1800 22 8374 (toll-free)

+91 22 6716 2200

All Other Enquiries +44 (0) 1928 534 050

Technical Support

North America +1 800 332 3331

Outside North America +44 (0) 1928 534 440

Thermo
SCIENTIFIC